

Display Report


Analysis Info

Analysis Name D:\Data\test\0519\gancaozaertong_99_01_1372.d
Method 1372.m
Sample Name gancaozaertong
Comment

Operator
Instrument bruker
amaZon SL

Acquisition Parameter

Ion Source Type	ESI	Ion Polarity	Positive	Alternating Ion Polarity	off
Mass Range Mode	UltraScan	Scan Begin	70 m/z	Scan End	1000 m/z
Capillary Exit	140.0 V	n/a	n/a	Trap Drive	50.6
Accumulation Time	2014 μ s	Averages	5 Spectra	Auto MS/MS	off

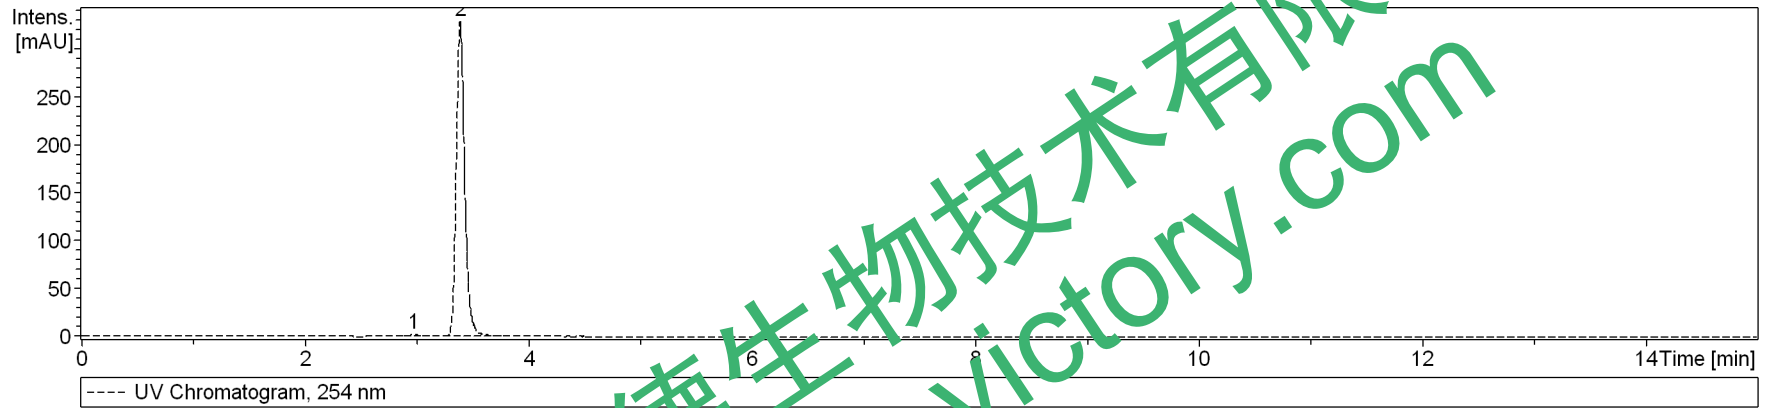

#	RT [min]	Area	Area Frac. %
1	3.0	11.602	0.7
2	3.4	1729.721	99.3

Display Report

Analysis Info

Analysis Name D:\Data\test\0519\gancaozaertong_99_01_1372.d
Method 1372.m
Sample Name gancaozaertong
Comment

Operator
Instrument bruker
amaZon SL

Acquisition Parameter

Ion Source Type	ESI	Ion Polarity	Positive	Alternating Ion Polarity	on
Mass Range Mode	UltraScan	Scan Begin	70 m/z	Scan End	1000 m/z
Capillary Exit	140.0 V	n/a	n/a	Trap Drive	50.6
Accumulation Time	2014 μ s	Averages	5 Spectra	Auto MS/MS	off

